

# Standards and Recommended Practices

## Approved SMPTE Recommended Practices

The Society approved three SMPTE Recommended Practices: RP 18-1991, Specifications for Test Film for Subjective Checking of 16-mm Motion-Picture Audio Projectors; RP 133-1991, Specifications for Medical Diagnostic Imaging Test Pattern for Television Monitors and Hard-Copy Recording Cameras; and RP 159-1991, Vertical Interval Time Code and Longitudinal Time Code Relationship. The practices are available from Society Headquarters for \$5.00 each.

## Proposed SMPTE Standard

A Proposed SMPTE Standard is published here for a trial period and public review: SMPTE 254, Motion-Picture Film (35-mm) — Manufacturer-Printed, Latent Image Identification Information. The proposal was previously published in the October 1990 issue of the *Journal* and is being republished because of extensive technical changes. The proposal will be submitted to the American National Standards Institute for approval as an American National Standard if no adverse comments are received from publication. Comments should be addressed to Sherwin H. Becker, Director of Engineering, at Society Headquarters prior to September 1, 1991. Copies of the proposal are available from Headquarters for \$10.00.

## Proposed SMPTE Recommended Practices

Also published for trial and comment are two Proposed SMPTE Recommended Practices: RP 131, Storage of Motion-

Picture Films; and RP 161, Logic Design for Decoding Digital Audio Control Words in D-1 Helical Data and Control Records. The proposals will be approved if no comments are received by September 1, 1991. Both practices are available from Headquarters for \$5.00 each.

## Reaffirmed American National Standard

Reaffirmation of an American National Standard sponsored by the Society was approved by the American National Standards Institute on March 22, 1991: ANSI/SMPTE 183-1985 (R1991), Motion-Picture Film — Measurement of Photoelectric Output Factor — Photographic Audio Level Test Films. Copies of the standard are available from the Society at \$8.00.

## American National Standards Withdrawn

A recommendation for withdrawal of two American National Standards was approved by the American National Standards Institute on March 22, 1991: ANSI V98.27M-1983, Video Recording — 1-in Type C Reference Recorders — Basic System and Transport Geometry Parameters; and ANSI V98.28M-1983, Video Recording — 1-in Type C Reference Tapes — Records. Withdrawal was initiated because no test tapes have been or are likely to be built that are readily available for sale, changes in mechanical tolerances are not included, and manufacturers are already manufacturing to tighter tolerances than those specified.

— *Sherwin H. Becker, Director of Engineering*

## **SMPTE Standards Subscription Service**

The Society provides a Standards Subscription Service to assist firms, libraries, and individuals in establishing and maintaining a complete and current file of approved American National Standards, SMPTE Recommended Practices, and SMPTE Engineering Guidelines in the motion-picture, television, and video magnetic recording fields. Through this service, the Society makes automatic distribution to standards subscribers of all new and revised standards, recommended practices, and guidelines that are approved during the calendar year in these fields.

For further information, write to: Standards Subscription Service, Engineering Dept., Society of Motion Picture and Television Engineers, 595 West Hartsdale Ave., White Plains, NY 10607.

## SMPTE RECOMMENDED PRACTICE

## Specifications for Test Film for Subjective Checking of 16-mm Motion-Picture Audio Projectors

RP 18-1991  
Revision of RP 18-1986

Page 1 of 2 pages

**1 Scope**

This practice describes a test film and a method for subjective checking and demonstrating 16-mm motion-picture projection and audio performance.

**2 Normative references**

The following documents contain provisions which, through reference in this text, constitute provisions of this practice. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this practice are encouraged to investigate the possibility of applying the most recent edition of the documents indicated below.

ANSI/SMPTE 10M-1985, Motion-Picture Film (16-mm) — Projector Usage

ANSI/SMPTE 41-1989, Motion-Picture Film (16-mm) — Photographic Audio Records — Prints

ANSI/SMPTE 109-1986, Motion-Picture Film (16-mm) — Perforated 1R

ANSI/SMPTE 112-1989, Motion-Picture Film (16-mm) — 100-Mil Magnetic Audio Record

ANSI/SMPTE 233-1987, Motion-Picture Film (16-mm) — Projectable Image Area

SMPTE RP 67-1989, Specifications for Buzz-Track Test Film for 16-mm Motion-Picture Audio Reproducers, Photographic Type

**3 Test film specifications**

3.1 Where applicable, the film shall contain the following sections:

**3.1.1 Audio samples**

(a) Dynamic wide-range orchestration to check reproduction of music.

(b) A recording of piano music having sufficiently sustained notes that a subjective assessment of wow and flutter can be made.

(c) Seven tones (nominally 50, 125, 500, 800, 2000, 3150, and 5000 Hz) recorded at normal program level.

(d) A section of male and female actors in dialog as a check for speech intelligibility and synchronization.

16-mm photographic audio version only:

(e) A section of buzz-track test film as specified in SMPTE RP 67-1989.

(f) Three sections of a 5-kHz tone to check for a compromise focus for the photographic audio record; sections one and three in the normal emulsion position and section two in a reverse emulsion position.

**3.1.2 Picture samples**

(a) General picture steadiness (vertical and horizontal).

(b) Uniform projected picture luminance.

(c) General picture quality such as sharpness and contrast.

3.2 Each film shall be provided with a leader and trailer. The main title shall include the issue number. Titles or subtitles, as appropriate, shall indicate the particular projector audio and/or picture characteristic to be tested by that portion of the film.

RP 18-1991

3.3 Each film shall be accompanied by an instruction sheet describing the procedure to be used for checking the projection equipment.

**4 Prints**

4.1 The film stock used shall be cut and perforated in accordance with long-pitch dimensions specified in ANSI/SMPTE 109-1986.

**Annex A (informative)  
Procedure****A.1 Method of use**

With the projector set up for projection of an audio picture print and the loudspeaker(s) properly located in accordance with the instructions furnished with the equipment, proceed as follows:

(a) Pre-set tone control(s) to normal, thread test film into projector, and set volume for comfortable loudness. If the audio optics have adjustable focus, adjust the focus to give the most satisfactory audio quality.

(b) Frame and focus picture for best overall screen image.

**A.2 Audio and visual qualities**

As the test sections are projected, observe the following:

(a) Listen for full range of orchestra and overall quality of audio. Note picture steadiness at top and sides. Note picture sharpness across the entire frame. White streaks above or below letters indicate travel ghost.

(b) Look for uniform picture brightness. Listen for smooth, even music; quaver indicates flutter.

4.2 The audio record dimensions shall comply with ANSI/SMPTE 41-1989 or ANSI/SMPTE 112-1989.

4.3 Color prints shall be made with the emulsion toward the lens for direct-projection viewing. The prints shall be in accord with ANSI/SMPTE 10M-1985 and ANSI/SMPTE 233-1987.

NOTE — Test films conforming to this practice are available from the Society of Motion Picture and Television Engineers.

(c) Silence or equal loudness of the two tones of the buzz-track shows correct lateral positioning of the audio producer (photographic record only).

(d) In the photographic audio version, three successive tones (5000 Hz) are included to permit detection of correct audio focus. Emulsion position is reversed for the second (middle) tone. (To compensate for prints which may be projected emulsion to the lens or emulsion away from the lens, a compromise position of the photographic audio-focusing optics must be determined so that the audio level results in equal loudness between the two positions. The difference between the two positions can be considered as the mid-point of the film, 0.0035 in (0.089 mm) below the surface.)

(e) Seven tones are provided having the frequencies of 50 to 5000 Hz. All should reproduce well.

(f) Listen for natural quality of the audio and proper lip synchronization of voices.

# SMPTE RECOMMENDED PRACTICE

RP 133-1991  
Revision of RP 133-1985

## Specifications for Medical Diagnostic Imaging Test Pattern for Television Monitors and Hard-Copy Recording Cameras



Page 1 of 6 pages

### 1 Scope

This practice describes the format, dimensions, and contrast required to make diagnostically significant measurements of the display and camera system resolution for both digital and analog monochrome signal sources. (See note.) The practice provides users of medical diagnostic imaging systems with a comprehensive test pattern for day-to-day operational checks and adjustments of focus, brightness and contrast, resolution response, mid-band streaking, uniformity, and linearity of viewing monitors and hard-copy recordings. This practice is not intended to create a standard for image characteristics such as resolution, geometry and linearity, uniformity, phosphor defects, etc. However, use of the pattern is encouraged as an appropriate tool for evaluating the measurement and specification of such image characteristics.

### 2 Description

#### 2.1 Pattern

A reproduction of the test pattern is shown in figure 1. Figure 2 is a drawing of the pattern for reference to the following text:

#### 2.2 Background

The background is presented at 50% of maximum white to obtain an approximate average picture level (APL) of 50% (figure 2 [1]).

#### 2.3 Crosshatch pattern

This pattern allows verification of linearity, either by using a straightedge or by overlaying or projecting a perfect reference image (Ball chart) (figure 2 [2]).

#### 2.4 Resolution pattern

Three zones of vertical and horizontal, high-contrast bar patterns are placed in five locations (four corners and the center). The modulation depth of the pattern is 100%. Placement of the patterns facilitates comparison of the resolution in the center and in the corners of the screen (figure 2 [3]). A detailed view of the resolution pattern is shown in figure 3.

#### 2.5 Low-contrast imaging resolution

Three zones of vertical and horizontal, low-contrast, equally-spaced bars are located next to the patterns described in 2.4. The modulation depth of these areas is 1%, 3%, and 5%. This is the most sensitive test for various types of imaging noise (figure 2 [4]).

#### 2.6 Gray step pattern

Blocks of specified signal amplitude, representing 0% to 100% of the input signal in steps of 10%, allow measurements of the response characteristics of the viewing monitors and hard copy (figure 2 [5]).

##### 2.6.1 Small-contrast changes

Small-contrast changes of 5% of the input signal are superimposed on a 0% background, and a 95% value is superimposed on a 100% maximum signal background to allow quick verification that all available gray-scale information can be presented in the image to be displayed (figure 2 [6]).

#### 2.7 White window and black window

During display of these patterns, the display or recording device signal stays relatively long in one state (black or white). These large areas of maximum contrast facilitate detection of mid-band streaking (poor low-frequency response), video amplifier ringing or overshoot, deflection interference, and halo (figure 2 [7] and [8]).

RP 133-1991

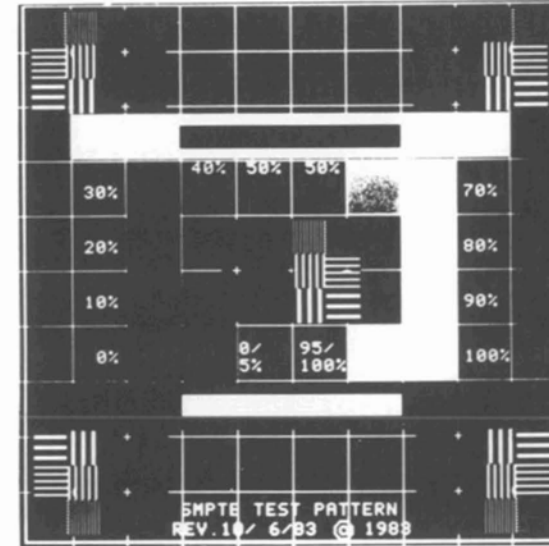


Figure 1 – Video hard-copy camera image of test pattern

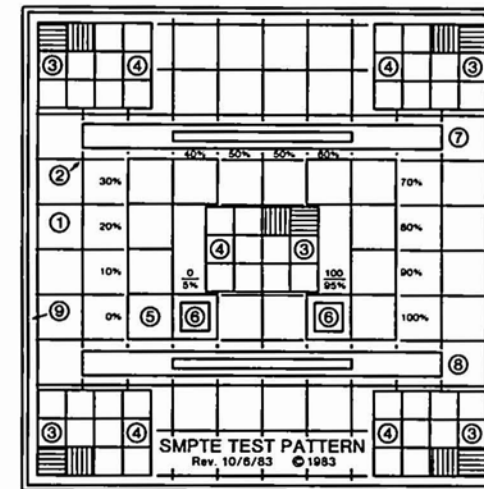


Figure 2 – Schematic drawing of test pattern in a square format

**2.8 Picture border**

A line is placed around the outside of the pattern that defines the full extent of the pattern (figure 2 [9]).

**3 Format**

**3.1** The test pattern (figure 2) and the following paragraphs shall represent a recommended implementation of the pattern. Specific information for digital implementation is given in table 1.

**3.2** The middle gray background is used to isolate the gray-scale and center resolution pattern from interference by adjacent patterns.

**3.3** Crosshatch lines in the horizontal direction shall be two raster lines wide, and in the vertical direction, lines shall be of a width equal to two raster lines. The intensity of the line shall be 75% of the maximum signal. The patterns shown consist of square spaces equal to 10% of the raster height. Rectangular aspect ratios and different numbers of scan lines may require fractional spaces (see figure 4). Fractional spaces, if required, should be at the edges of the pattern.

**3.4** The high-contrast resolution patterns of lines in the vertical direction are divided into three zones of different spatial frequencies with the highest frequency pattern in the four corners. The center pattern is oriented with its high-contrast, high-resolution pattern in the upper-right corner (see figure 3). Modulation of the high-contrast pattern is 100%.

**3.5** It is recommended that the high-contrast middle spatial frequency zone of the horizontal resolution patterns (which are placed in the four corners of the test pattern) should represent the corner resolution specified by the manufacturer for the system being evaluated. The high-contrast middle frequency zone of the resolution pattern (in the center of the test pattern) should represent the central display resolution as specified by the manufacturer of the system being evaluated. The lower frequency pattern in each of these five high-contrast test patterns should be 75% of the resolution specified by the manufacturer for the area in which the resolution pattern is located. The high-contrast highest frequency pattern should be 125% of the resolu-

tion specified by the manufacturer for the area in which the pattern is located.

**3.5.1** Vertical resolution patterns are limited to three arrangements; one line off and one line on, two lines off and two lines on, and three lines off and three lines on.

**3.6** For digital systems, the spatial frequency of the bar patterns is limited to increments of one pixel size. Thus, it is recommended that one pixel on and one pixel off be used for the highest resolution zone and three pixels on and three pixels off be used for the lowest resolution zone.

**3.7** Low-contrast patterns repeat the format of the high-contrast patterns except the spatial frequency in all three zones is equal to that of the above middle zone; however, in one zone the modulation is 1% (i.e., white equals 51% and black equals 50%). In the middle zone, the modulation is 3% (51% and 48%), while in the last zone, it is 5% (53% and 48%). The arrangement of patterns is symmetrical, with the lowest-contrast zones closest to the corners.

**3.8** A rectangular area 40% of the picture height is used to display at least 10 steps of luminance from white to black. Thus, the resolution performance is evaluated at the proper dynamic range of the image as it is used for operation for both viewing monitor and film hard copy. The individual blocks are intended to be measured with a spot photometer or optical densitometer, and they are concentrated in the middle of the screen to avoid shading caused by off-axis effects in the CRT or optical system.

**3.9** Small contrast changes in the blocks next to the white and black ends of the gray scale consist of a 5% maximum signal patch superimposed on 0% (i.e., black) and a 95% maximum signal patch superimposed on 100% (i.e., white) to permit fine tuning of contrast and brightness controls to verify that all shades of gray present in the signal can be perceived in the image. The size of the inset shall be 5% of the picture height.

**3.10** The white and black window patterns should have a height equal to 8% of the picture height centered in one square of the crosshatch with the length starting one square away from the left edge and continuing up to the last square on the right.

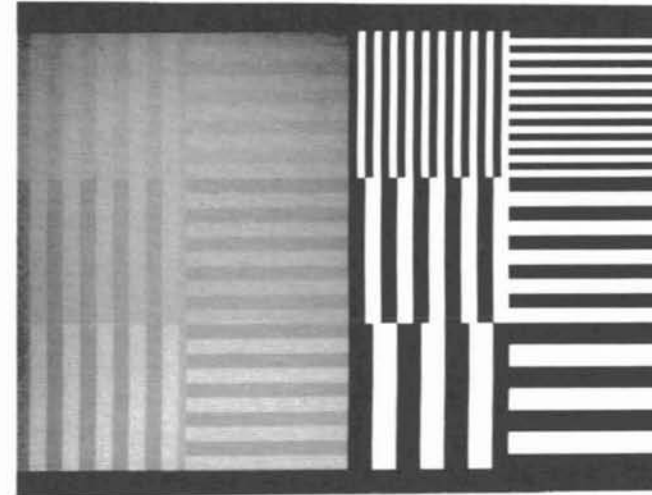


Figure 3 – Detail of digitally-generated resolution pattern portion of test pattern showing high- and low-contrast portions

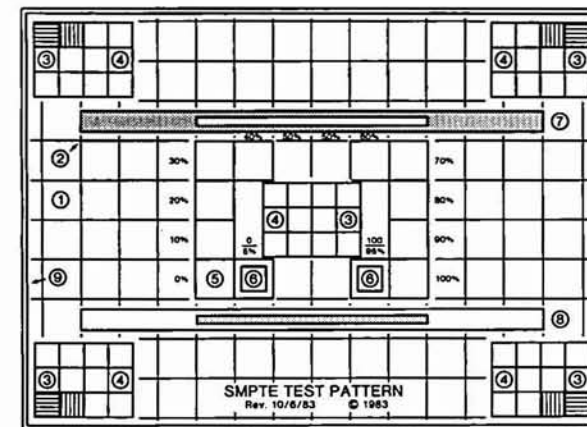


Figure 4 – Schematic drawing of test pattern in rectangular format

Table 1 – Test image pixel sizing for digital imaging systems

	Percent video signal	Percent of picture height	Array size			
			256x 256	320x 320	512x 512	1024x 1024
2. Crosshatch – vertical spacing	75%	10%	25	32	50	102
horizontal spacing		10%	25	32	50	102
line width			2	2	2	2
3. High-contrast resolution –						
Each block		6.25%	16	20	32	64
Low frequency – 3 pixels on, 3 pixels off						
Mid frequency – 2 pixels on, 2 pixels off						
High frequency – 1 pixel on, 1 pixel off						
Contrast all the same – 0-100%						
4. Low-contrast resolution –						
Each block		6.25%	16	20	32	64
Frequency – 2 pixels on, 2 pixels off						
Contrast – low – 50-51%						
medium – 48-51%						
high – 48-53%						
5. Gray scale pattern		10%	25	32	50	102
6. Small contrast changes	5% and 95%	5%	12	16	25	51
7. & 8. White and black window	5% and 95%					
Surround bar – height		8%	20	26	40	82
– width		80%	205	256	410	820
Inset bar – height		4%	20	13	20	41
– width		40%	102	128	205	410
9. Border – width	75%	0.5%	2	2	3	5
– inset		1%	2	3	5	10

NOTE – If other than a square format is used, the four resolution patterns should be placed in the corner of the display.

3.10.1 The inset window shall be 4% of the picture height and 1/2 the length of the background.

3.10.2 In the upper window pattern, the background shall be equal to 95% of the maximum signal, and the window shall be 5% of the maximum signal. In the lower window, the opposite intensities shall be used.

3.11 The border shall be a line inset by 1% of the picture height and shall be 0.5% of the picture height or 2 TV lines or pixels, whichever is larger. The border shall be 75% of the peak white signal.

3.12 All lettering shall be displayed at the 100% signal level. The numbers around the gray-scale

are to be kept as small as legibility will allow. It has been found that the percent signs are especially valuable in focusing.

3.13 For systems with video-invert capability, the pattern should invert symmetrically. If the inversion operates about the midpoint of the video signal, the 50% signal background of the pattern should have the same brightness level or film density.

NOTE – The test pattern was initially designed for certification of monochrome systems; however, it can be utilized equally well for color displays and monitors in the RGB or encoded mode of operation.